



RIGEL MEDICAL
GMC-INSTRUMENTS GROUP

How do I Calibrate the Zero offset on my FloTest/F2?





RIGEL MEDICAL

FloTest

Before the Measurement

1. Remove the protection caps from both sides of the flow measurement channel
2. Allow the FloTest/F2 to warm-up for about 15 minutes
3. Press the Menu tab, located on the top left hand side of your screen
4. Select the "Zero Calibration" option
5. Press the "Start calibration" tab to begin the calibration
- 6.

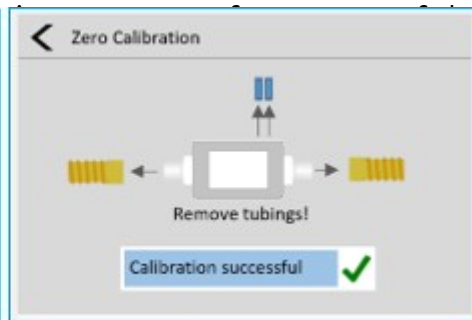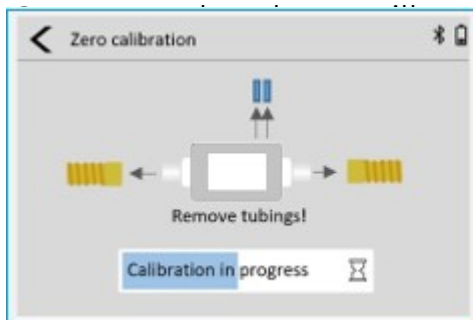

Please note the following:


- For a short moment after the zero calibration, allow the instrument to settle, and the zero value will be displayed
- Ensure that the 10 to 15 minutes warm up time is allowed, or your

calibration may be unsuccessful. This should be performed in the environment that you intend to perform your testing.

- During a zero calibration it is important that no pressure or flow is applied to any connector and that the protection caps are removed

Calibration failed

The device is **not** ready to use.



If the calibration failed, ensure that all tubes and the protection caps are removed, and that there is no pressure or flow in the channel during zero offset calibration. In environments with high turbulence, close one of the flow ports using a protection cap.

The Accuracy will remain valid within the following conditions:

- Between 10°C and 30°C (channel temperature)
- Between 950 hPa and 1250 hPa (hectoPascals)
- The zero offset calibration performed after the required warm-up period
- For measurements performed within 4 h after last zero offset calibration at same ambient conditions

If you require more help, please contact us at
<https://www.seaward.com/gb/enquire/>.